


Keysight Technologies

7 Hints That Every Engineer Should Know When Making Power Measurements with Oscilloscopes

Application Note

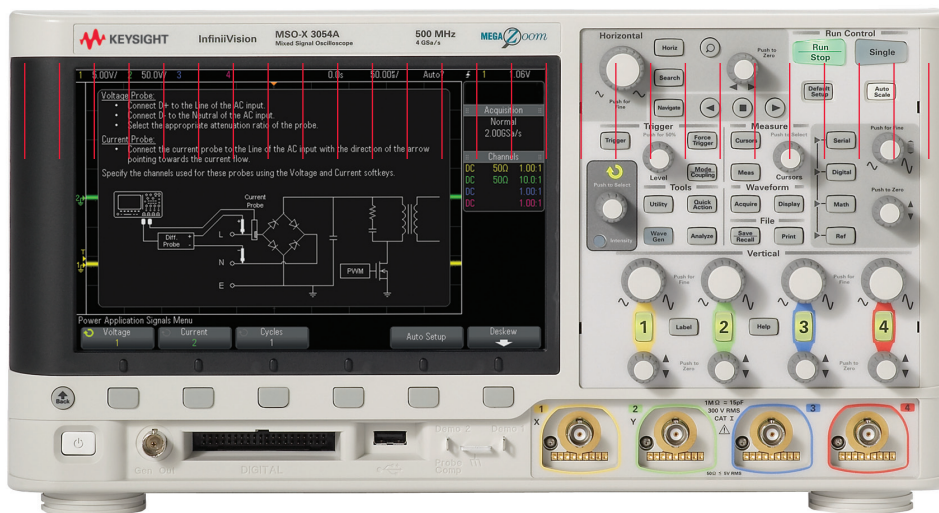

Seven Hints for Making Power Measurements with Oscilloscopes

Achieving maximized measurement dynamic range

- 1) Use averaging to increase measurement resolution
- 2) Use high-resolution acquisition to increase measurement resolution
- 3) Use AC coupling to remove DC offset
- 4) Bandwidth limiting with the oscilloscope and probes

Probing to optimize signal integrity

- 5) Use differential probes for safe and accurate floating measurement
- 6) Avoid probing accessories that couple radiated power
- 7) Select probes that avoid the scope's most sensitive settings

1st Hint: Use averaging to increase measurement resolution

For some power-measurement applications, you need to measure a large dynamic range of values; and at the same time you need fine resolution to measure small changes in a parameter. Rather than resorting to a high-resolution digitizer, you can use alternative acquisition methods to reduce random noise and increase the effective dynamic range of your measurements. Two methods are average and high-resolution acquisition.

Averaging requires a repetitive signal. The algorithm works by averaging the points in each time bucket across multiple acquisitions. This reduces random noise, and gives you better vertical resolution.

How many averages are needed per extra bit of vertical resolution? You get one extra bit of vertical resolution for every four averages of the samples. It works like this:

- Number of bits increased = $0.5 \log_2 N$
- N = the number of samples averaged
- For example, averaging 16 samples will yield an improvement of:
- Number of bits = $0.5 \log_2 16 = 2$
- Therefore, the effective vertical resolution is $8 + 2 = 10$ bits.

This algorithm maximizes out at ~12 bits of vertical resolution because other factors, such as vertical gain or offset accuracy of the oscilloscope, begin to dominate. The advantage of averaging mode is that it does not limit the scope's real-time bandwidth. The disadvantages of averaging mode are that it requires a repetitive signal and it slows waveform update rate.

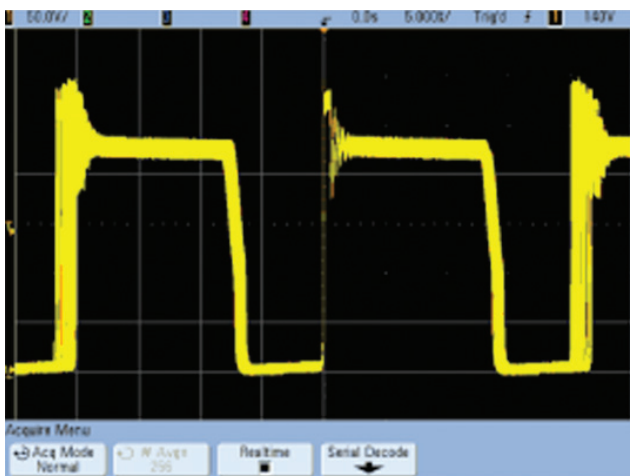


Figure 1. Vds of a switching power supply captured with normal acquisition

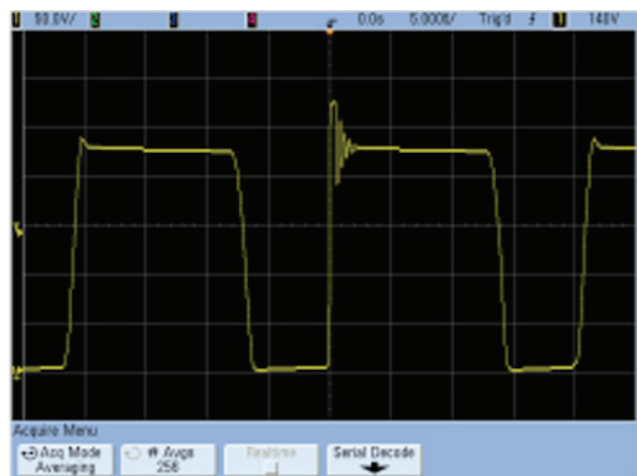


Figure 2. Vds captured in normal averaging mode

2nd Hint: Use high-resolution acquisition to increase measurement resolution

The second noise reduction method, one that does not require a repetitive signal, is called high-resolution mode. Modern oscilloscopes such as the Keysight Technologies, Inc. InfiniiVision 3000 X-Series provide 8-bit vertical resolution in normal acquisition mode (like most other digitizing oscilloscopes). However, like averaging, high-resolution mode also yields up to 12 bits of vertical resolution.

Instead of averaging points from multiple acquisitions in a single time bucket, high-resolution mode averages sequential points within the same acquisition. In high-resolution mode, you cannot directly control the number of averages as you can in averaging mode. Instead, the number of extra bits of vertical resolution is dependent on the time/division setting of the scope.

When operating at slow time-base ranges, the oscilloscope serially filters sequential data points and maps the filtered results to the display. Increasing the memory depth of on-screen data increases the number of points averaged together. High-resolution mode has less effect at faster sweep speeds, where the number of on-screen points captured is fewer. It has a significant effect at slower sweep speeds, where the number of on-screen points captured is larger.

3rd Hint: Use AC coupling to remove DC offset

If you are focusing on a signal's ripples, you won't care much about its DC offset. Normally, ripple and noise are small in relation to the power-supply voltage. If you use your scope's dynamic range quantifying this offset, it won't be available to give insight into smaller signal details. Setting the scope's coupling to "AC" will remove the DC offset from your measurements, maximizing the linearity and dynamic range of your measurements.

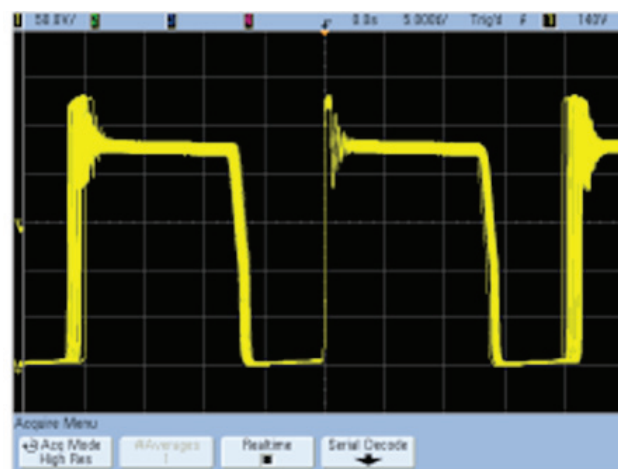


Figure 3: V_{ds} captured in high-resolution mode

4th Hint: Bandwidth limiting with the oscilloscope and probes


This is a simple, but often overlooked, way to reduce noise and increase dynamic range. Power signal content tends to be much lower (on the order of kHz to 10s of MHz) than the nominal bandwidth of the scope. Additional bandwidth will add no signal information, but will introduce additional noise to your measurements.

Most oscilloscopes have dedicated hardware filters for just this application – typically 20 to 25 MHz low-pass. A benefit of hardware filters over software-based filters is that there is no impact on the scope's update rate.

Another approach is to use your probes to limit bandwidth. The bandwidth of a measurement chain is limited by the “weakest link.” A 500 MHz oscilloscope probe with a 10 MHz probe will have a bandwidth of 10 MHz. Keysight offers a wide variety of passive, active current, and differential probes with a bandwidth that will fit your specific measurements.

5th Hint: Use differential probes for safe and accurate floating measurements

The ground lead on a scope probe is connected to the chassis through the shell of the BNC connector. For safety purposes, the chassis of the scope connects to earth-referenced ground through the ground tap of the power cord. The scope's grounding can cause conflict with the way the power supply is grounded. Many of the signals of interest are referenced to a potential other than ground (floating). Power-supply designers use several techniques to overcome this measurement limitation.

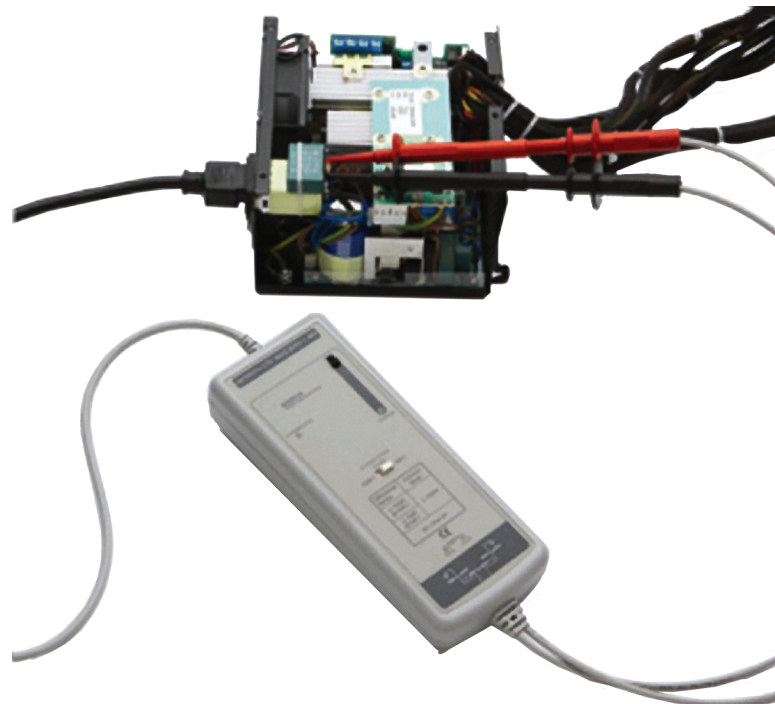

The most commonly-used method is to “float” (isolate) the scope, either by cutting the protective ground tab in the power cord or using an isolation transformer in the power line. This is a dangerous practice because of the potential high voltage presented on the scope chassis. In addition, the measurements from a floating scope can lead to an inaccurate measurement result.


Another technique used for measuring a floating power-supply signal is subtracting channel A and channel B using two single-ended voltage probes. Two input channels and probes are used to measure the signal node of interest. Then, using the waveform math function on the scope, two channels are electrically subtracted, giving a trace of the difference signal.

This technique is relatively safe, since the scope remains grounded. However, it is limited to measurements where the common mode signal is relatively small, as the common mode rejection ratio is low – approximately less than 20 dB (10:1) -because of the gain mismatches between the two probes input channels being used.


The best solution for making a safe and accurate floating measurement is to use a differential probe or differential amplifier. Differential probes offer a high common mode rejection ratio, typically as high as 80 dB or 10,000:1 or higher, allowing you to measure a small differential signal riding on high common-mode signals with decent accuracy and high sensitivity. Use a differential probe with sufficient dynamic range and bandwidth for your application to make a safe and accurate floating measurement.

6th Hint: Avoid probing accessories that couple radiated power

Be careful in which probing accessories you use. The 15-cm-long ground lead and hook tip that typically come the standard with general-purpose passive probes may pick up noise generated by the power supply or other devices. In addition, inductive loading caused by a long ground connection often adds ringing to the signal you're measuring.

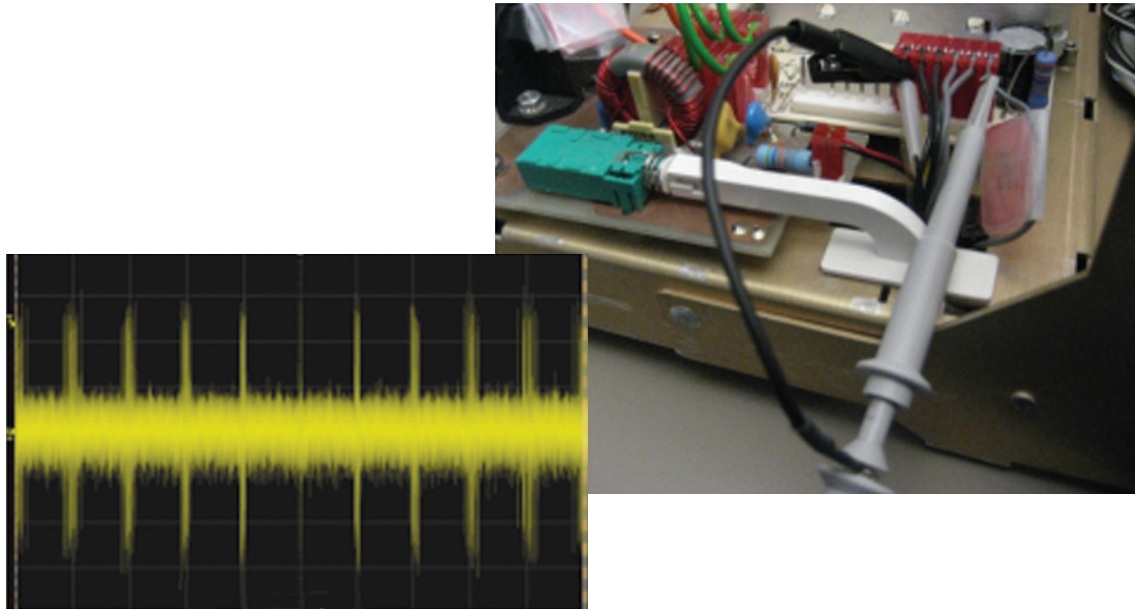


On the other hand, the smaller probe tip and shorter ground connection--such as from using a BNC adapter on the board or a bayonet type of ground lead--significantly reduces noise picked up. It accomplishes this performance by minimizing the loop of the connections and also reducing inductive loading.

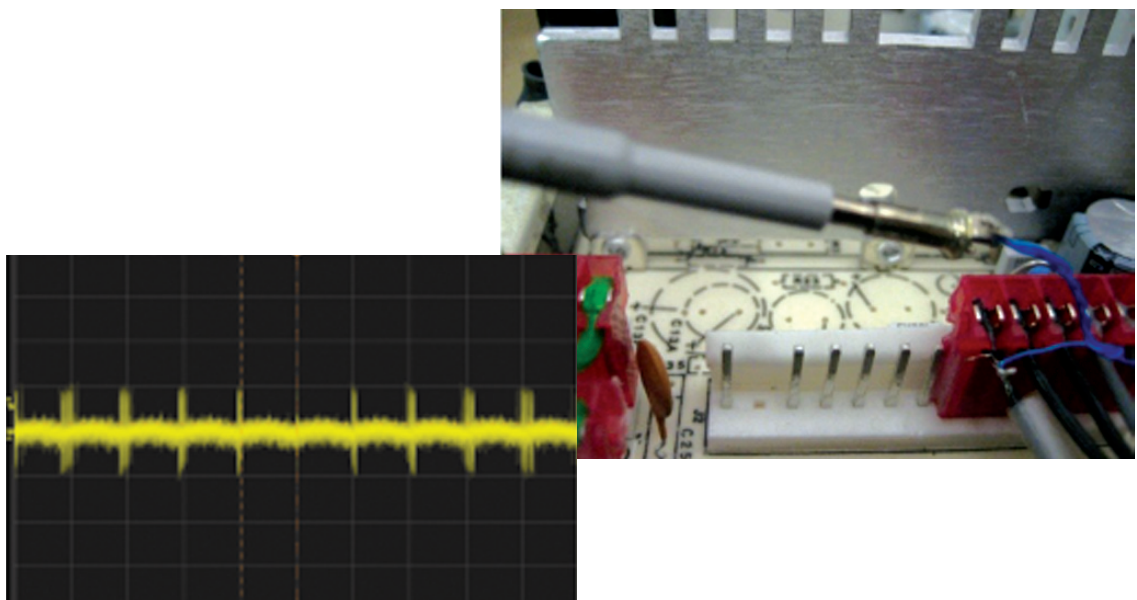

7th Hint: Select probes that avoid the scope's most sensitive settings

If you are measuring the amplitude of ripple and noise on your power supply, you may need to use a scope at or near its most sensitive V/div setting. This will be at the edge of its amplifiers' performance envelope. Your instrument will perform within specification, but you may not get its "base case" performance.

Consider using a 1:1 probe, rather than using the standard 10:1 passive probe that was shipped with your instrument. With a 10:1 probe, not only is the oscilloscope's baseline noise floor increased by a factor of 10, but the minimum V/div setting of scope is also ten times higher than with a 1:1 probe. This reduction of SNR will diminish the dynamic range of your measurements. A less-attenuated probe, as long as you do not exceed the scope's maximum input voltage, can yield superior signal integrity.

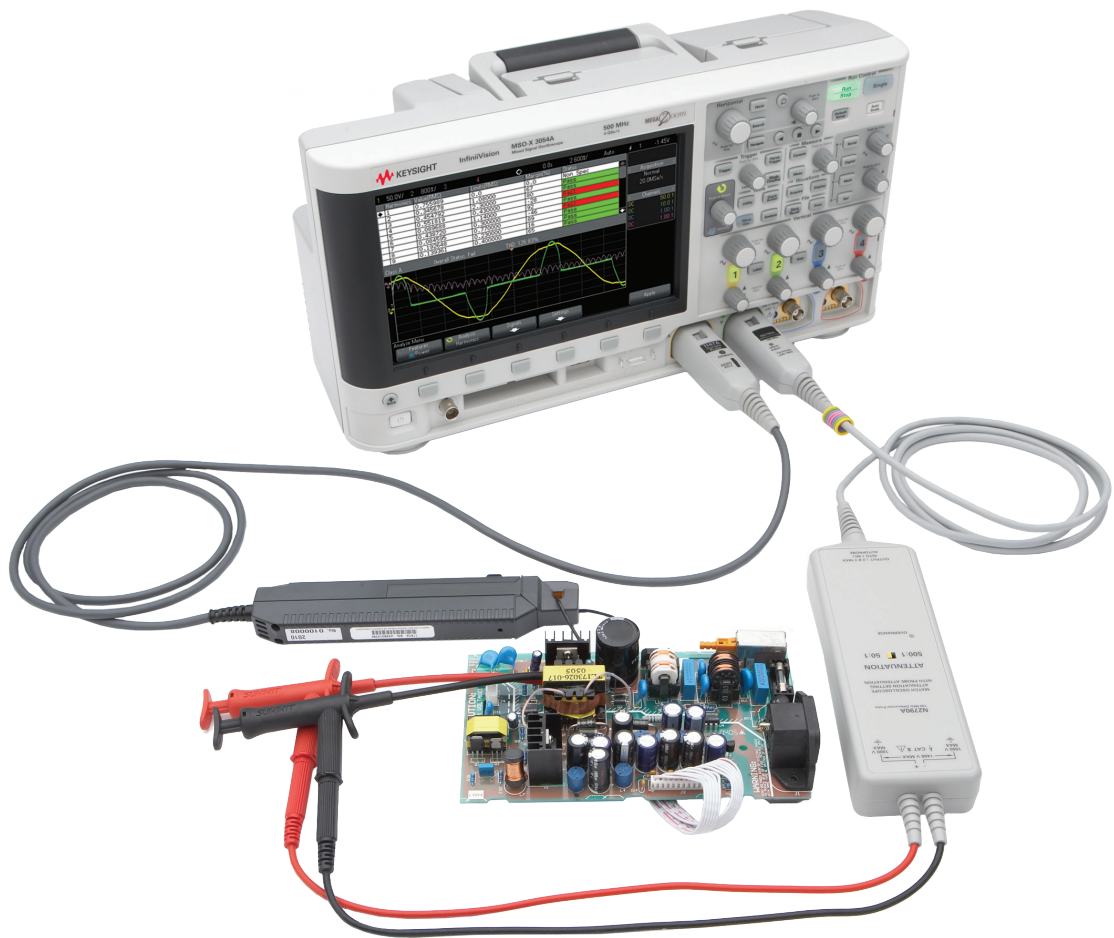

myKeysight

myKeysight

www.keysight.com/find/mykeysight

A personalized view into the information most relevant to you.



www.axiestandard.org

AdvancedTCA® Extensions for Instrumentation and Test (AXIe) is an open standard that extends the AdvancedTCA for general purpose and semiconductor test. Keysight is a founding member of the AXIe consortium.



www.lxistandard.org

LAN eXtensions for Instruments puts the power of Ethernet and the Web inside your test systems. Keysight is a founding member of the LXI consortium.



www.pxisa.org

PCI eXtensions for Instrumentation (PXI) modular instrumentation delivers a rugged, PC-based high-performance measurement and automation system.



www.keysight.com/quality

Keysight Technologies, Inc.
DEKRA Certified ISO 9001:2008
Quality Management System

Keysight Channel Partners

www.keysight.com/find/channelpartners

Get the best of both worlds: Keysight's measurement expertise and product breadth, combined with channel partner convenience.

www.keysight.com/find/power-meas

For more information on Keysight Technologies' products, applications or services, please contact your local Keysight office. The complete list is available at: www.keysight.com/find/contactus

Americas

Canada	(877) 894 4414
Brazil	55 11 3351 7010
Mexico	001 800 254 2440
United States	(800) 829 4444

Asia Pacific

Australia	1 800 629 485
China	800 810 0189
Hong Kong	800 938 693
India	1 800 112 929
Japan	0120 (421) 345
Korea	080 769 0800
Malaysia	1 800 888 848
Singapore	1 800 375 8100
Taiwan	0800 047 866
Other AP Countries	(65) 6375 8100

Europe & Middle East

Austria	0800 001122
Belgium	0800 58580
Finland	0800 523252
France	0805 980333
Germany	0800 6270999
Ireland	1800 832700
Israel	1 809 343051
Italy	800 599100
Luxembourg	+32 800 58580
Netherlands	0800 0233200
Russia	8800 5009286
Spain	0800 000154
Sweden	0200 882255
Switzerland	0800 805353
	Opt. 1 (DE)
	Opt. 2 (FR)
	Opt. 3 (IT)
United Kingdom	0800 0260637

For other unlisted countries:
www.keysight.com/find/contactus
(BP-06-23-14)